

# The $\alpha$ 1-Microglobulin Turbidimetric Immunoassay Kit

Catalogue number: 51900

For the quantitative determination of  $\alpha$ 1-Microglobulin  
in human serum and plasma

This package insert must be read in its entirety before using this product  
Use only the current version of product data sheet enclosed with the kit

Website: [www.immunodiagnostics.com.hk](http://www.immunodiagnostics.com.hk)

E-mail: [info@immunodiagnostics.com.hk](mailto:info@immunodiagnostics.com.hk)

Tel: (+852) 3502 2780

Fax: (+852) 3502 2781

**FOR RESEARCH USE ONLY  
NOT FOR USE IN DIAGNOSTIC PROCEDURES**

Version: 1.1



## TABLE OF CONTENT

Content	Page
INTRODUCTION	1
PRINCIPLE OF THE ASSAY	1
REAGENTS SUPPLIED	2
OTHER MATERIALS REQUIRED, BUT NOT PROVIDED	2
STORAGE	2
SAMPLE HANDLING	2
ASSAY PROCEDURE	3
TYPICAL STANDARD CURVE	3
CALCULATION	4
ASSAY CHARACTERISTICS	4

## PACKING SPECIFICATION

Cat. No.	Size	Approximately tests
51900-05	R1: 15ml, R2: 5ml	100
51900-10	R1: 30ml, R2: 10ml	200
51900-20	R1: 60ml, R2: 20ml	400
51900-50	R1: 150ml, R2: 50ml	1000
51900-100	R1: 300ml, R2: 100ml	2000

## INTRODUCTION

$\alpha$ 1-Microglobulin (A1M), also known as Protein HC, is a type of small globular protein containing 167 amino acids, which can be found in bloodstream and extravascular tissues of all organs. It is produced mainly in the liver and is broken down in the kidney. This low molecular weight protein can be filtered by the glomerulus and reabsorbed and catabolized by the proximal tubular cells.

The level of A1M is useful in screening for tubular abnormalities and detection of chronic asymptomatic renal tubular dysfunction. In healthy subjects, the concentration of A1M is < 30 mg/L in serum, or the ratio of A1M and creatinine in the urine is over 0.7 mg/mmol. Higher than this range is indicative of renal dysfunction, including acute kidney failure, glomerular disease and diabetic nephropathy?

IMD A1M PETIA kit can accurately measure A1M in human serum, plasma and urine samples.

## PRINCIPLE OF THE ASSAY

This assay is a turbidimetric immunoassay for the quantitative measurement of A1M in human serum and plasma. A standard or sample is added into a cuvette and mixed with the reaction buffer R1. After a short incubation, the test reagent R2, which is a suspension of microparticles coated with A1M antibodies, is added into the cuvette and mixed. The presence of A1M in the standard or sample causes the immune-particles to aggregate. The extent to which the microparticles aggregate is quantified by the amount of light scattering measured as absorbance by a chemistry analyzer. The concentration of A1M in unknown samples can be interpolated from a reference curve using the standards provided.

## **REAGENTS SUPPLIED**

R1 – Reaction buffer, a ready-to-use buffer solution containing salt, polyether compound and preservative

R2 – Test reagent, a ready-to-use suspension of polymer microparticles coated with rabbit anti-A1M polyclonal antibodies in storage buffer

## **OTHER MATERIALS REQUIRED, BUT NOT PROVIDED**

1. Clinical chemistry analyzer
2.  $\alpha$ 1-Microglobulin Calibrator (provided separately, Cat. #51900-S1)
3.  $\alpha$ 1-Microglobulin Control (optional, provided separately, Cat. #51900-C1)
4. Deionized water
5. Analyzer-specific reagent containers for R1 and R2

## **STORAGE**

The kit should be stored at 2-8°C upon receipt. Once opened, the reagents may be stored at 2-8°C for up to 4 weeks.

## **SAMPLE HANDLING**

This kit can be used to determine A1M in human serum and plasma samples. Blood specimens should be collected aseptically into appropriate tubes. Plasma should be prepared by standard techniques for laboratory testing. The prepared specimens should be stored in closed vessels. If the assay cannot be performed within 24 hours or specimens are to be shipped, the specimens should be frozen at -20°C or below. For long-term storage of specimens, -70°C or below is recommended. To avoid freeze-thaw cycles, specimens should be aliquoted. Do not use hemolyzed, hyperlipemic, heat-treated or contaminated specimens. No dilution of the sample is required in this assay.

## ASSAY PROCEDURE


Assay procedures may vary depending on the automated chemistry analyzer to be used. A general example of assay procedures is stated as follow:

1. Dispense 150µl of R1 into a clean cuvette
2. Add 1.5µl of sample and incubate at 37°C for 5 minutes
3. Further add 50µl of R2
4. Read change of absorbance at Main Wavelength 570 nm for 8 minutes after the addition of R2
5. Calculate the concentration of A1M in unknown sample by interpolation from a reference curve using the standards provided

## TYPICAL STANDARD CURVE

The following standard curve is provided for demonstration only. A standard curve should be generated for each assay.

A1M (mg/L)	Absorbance
0	-0.0098
6	0.0450
12	0.0950
25	0.2185
50	0.3345
100	0.4376

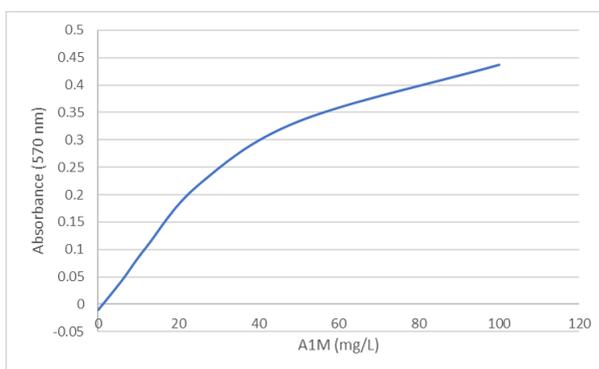

## CALCULATION

1. Subtract the absorbance of the blank from that of standards and samples.
2. Generate a standard curve by plotting the absorbance obtained (y-axis) against A1M concentrations (x-axis). The best fit line can be generated with any curve-fitting software by regression analysis. 4-parameter curve fitting can be used for calculation.
3. Determine A1M concentration of samples from standard curve.

## ASSAY CHARACTERISTICS

### A. Sensitivity

The sensitivity is defined as the lower limit of detection and is estimated as the mean of the blank sample plus three times the SD obtained from the blank sample. The sensitivity of A1M assay is 0.181mg/L.

### B. Precision

The precision of the A1M assay is < 5% CV. Two samples consisting of serum based panels were assayed 20 times separately.

Sample	Mean A1M (mg/L)	SD (mg/L)	CV
Panel 1	17.7	0.2	1.20%
Panel 2	32.4	1.0	3.00%

### C. Linearity

The A1M assay is linear between 6 mg/L to 100 mg/L.

### D. Interference

No interference was detected with hemoglobin up to 5 g/L, conjugated bilirubin up to 300 mg/L, free bilirubin up to 300 mg/L, and up to 5g/L lipid emulsion.