

# Mouse GDF-15 ELISA Kit

(Catalog Number: 32980)

For the quantitative determination of mouse GDF-15 concentrations in serum, plasma or cell culture supernate samples

## **IMD (Hong Kong)**

Address: Unit 513, 5/F, Biotech Centre 2, No. 11 Science Park West Avenue,  
Hong Kong Science Park, Sha Tin, Hong Kong

Website: [www.immunodiagnostics.com.hk](http://www.immunodiagnostics.com.hk)

Email: [info@immunodiagnostics.com.hk](mailto:info@immunodiagnostics.com.hk)

Tel: (+852) 3502 2780

## **IMD (Canada)**

Address: 3330 Bayview Avenue, Block #6, Toronto, M2M 3R8, Ontario, Canada

Email: [info@immunodiagnostics.ca](mailto:info@immunodiagnostics.ca)

Tel: +1-437-886-5136

## TABLE OF CONTENTS

Contents	Page
INTRODUCTION	1
PRINCIPLE OF THE ASSAY	1
INTENDED USE	1
REAGENTS SUPPLIED	1
OTHER MATERIALS REQUIRED, BUT NOT PROVIDED	1
STORAGE	2
PREPARATION OF REAGENTS	2
PREPARATION OF STANDARDS AND SAMPLES	2
ASSAY PROCEDURE	3
CALCULATION	3
TYPICAL STANDARD CURVE	4
ASSAY CHARACTERISTICS	4
REFERENCES	5
SUMMARY OF ASSAY PROCEDURE	5

## INTRODUCTION

Growth differentiation factor 15 (GDF-15) is a member of the transforming growth factor  $\beta$  cytokine superfamily, the protein is secreted as a 25 kDa disulfide linked dimer<sup>1</sup>. Circulating GDF-15 levels are associated with cancers, cardiovascular and kidney diseases<sup>2-4</sup>. GDF-15 regulates food intake, energy expenditure and body weight in response to metabolic and toxin-induced stresses<sup>5</sup>.

## PRINCIPLE OF THE ASSAY

This assay is a quantitative sandwich enzyme-linked immunosorbent assay (ELISA). The microtiter plate is pre-coated with a polyclonal antibody specific for mouse GDF-15. Standards and samples are pipetted into the wells and any mouse GDF-15 present is bound by the immobilized antibody. After washing away any unbound substances, a biotin labelled polyclonal antibody specific for mouse GDF-15 is added to the wells. After wash step to remove any unbound reagents, streptavidin-horseradish peroxidase conjugate (STP-HRP) is added. After the last wash step, an HRP substrate solution is added and color develops in proportion to the amount of mouse GDF-15 bound initially. The assay is stopped, and the optical density of the wells is determined using a microplate reader. Since the increases in absorbance are directly proportional to the amount of captured mouse GDF-15, the unknown sample concentration can be interpolated from a reference curve included in each assay.

## INTENDED USE

This Mouse GDF-15 ELISA kit is designed for quantification of mouse GDF15 in serum, plasma and cell culture supernate samples.

## REAGENTS SUPPLIED

*Each kit is sufficient for one 96-well plate and contains the following components:*

1. Microtiter Strips (96 wells), coated with a polyclonal antibody against mouse GDF-15, sealed
2. 10×Wash buffer, 50 mL
3. 5×Assay buffer, 20 mL
4. 100×Detection antibody solution, a biotin labelled polyclonal antibody against mouse GDF-15, 0.12 mL
5. Mouse GDF-15 standard, 250 pg of recombinant mouse GDF-15, lyophilized
6. 200×STP-HRP solution, 0.06 mL
7. Substrate solution, 12 mL, ready for use
8. Stop solution, 12 mL, ready for use

## OTHER MATERIALS REQUIRED, BUT NOT PROVIDED

1. Pipettes and pipette tips
2. 96-well plate or manual strip washer
3. Buffer and reagent reservoirs
4. Paper towels or absorbent paper
5. Plate reader capable of reading absorbency at 450 nm

Website: [www.immunodiagnosics.com.hk](http://www.immunodiagnosics.com.hk)

E-mail: [info@immunodiagnosics.com.hk](mailto:info@immunodiagnosics.com.hk)(HK) / [info@immunodiagnosics.ca](mailto:info@immunodiagnosics.ca)(Canada)

Tel: +852 3502 2780 (HK) / +1-437-886-5136 (Canada)

6. Distilled water or deionized water

### **STORAGE**

The kit should be stored at 2-8°C upon receipt, and all reagents should be equilibrated to room temperature before use. Remove any unused antibody-coated strips from the mouse GDF-15 microtiter plate, return them to the foil pouch and re-seal. Once opened, the strips may be stored at 2-8°C for up to one month.

### **PREPARATION OF REAGENTS**

*Bring all reagents and materials to room temperature before assay.*

#### **A. 1×Assay buffer**

Prepare 1×Assay buffer by mixing the 5×Assay buffer (20 mL) with 80 mL of distilled water or deionized water. If precipitates are observed in the 5×Assay buffer bottle, warm the bottle in a 37°C water bath until the precipitates disappear. The 1×Assay buffer may be stored at 2-8°C for up to one month.

#### **B. 1×Wash buffer**

Prepare 1×Wash buffer by mixing the 10×Wash buffer (50 mL) with 450 mL of distilled water or deionized water. If precipitates are observed in the 10×Wash buffer bottle, warm the bottle in a 37°C water bath until the precipitates disappear. The 1×Wash buffer may be stored at 2-8°C for up to one month.

#### **C. 1×Detection antibody solution**


Spin down the 100×Detection antibody solution briefly and dilute the desired amount of the antibody 1:100 with 1×Assay buffer, 100 µL of the 1×Detection antibody solution is required per well. Prepare only as much 1×Detection antibody solution as needed. Return the 100×Detection antibody solution to 2-8°C immediately after the necessary volume is removed.

#### **D. 1×STP-HRP solution**

Spin down the 200×STP-HRP solution briefly and dilute the desired amount of the 200×STP-HRP solution 1:200 with 1×Assay buffer, 100 µL of the 1×STP-HRP solution is required per well. Prepare only as much 1×STP-HRP solution as needed. Return the 200×STP-HRP solution to 2-8°C immediately after the necessary volume is removed.

### **PREPARATION OF STANDARDS AND SAMPLES**

**Mouse GDF-15 Standards:** Reconstitute the lyophilized standard with 1 mL of 1×Assay buffer to generate a standard stock solution of 250 pg/mL. Allow the standard to sit for 10 minutes with gentle agitation prior to making dilutions. Pipette 500 µL of 1×Assay buffer to 125, 62.5, 31.2, 15.6, 7.8, 3.9 pg/mL tubes. Use the standard stock solution to produce a serial dilution as shown below.

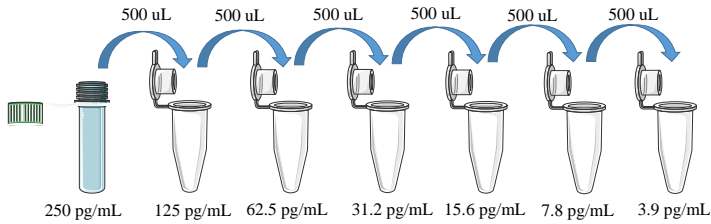

1×Assay buffer serves as the zero standard (0 pg/mL). The reconstituted standard stock should be aliquoted and stored at -80°C for up to one month. Avoid repeating freezing/thawing cycles. Please do not store the diluted standard solutions.

**Sample Preparation:**

Serum or plasma sample generally requires a **10-fold** dilution in the 1×Assay buffer. It is recommended that the users establish their own dilution factors based on the concentration range of their samples.

**ASSAY PROCEDURE**

*It is recommended that all standards and samples be assayed in duplicate.*

1. Add 100 µL of standard or sample per well, incubate at room temperature for 2 hours.
2. Discard the content and tap the plate on a clean paper towel to remove residual solution in each well. Add 300 µL of 1×Wash buffer to each well and incubate for 1 minute. Discard the 1×Wash buffer and tap the plate on a clean paper towel to remove residual wash buffer. Repeat the wash step for a total 3 washes.
3. Add 100 µL of 1×Detection antibody solution to each well, incubate at room temperature for 1 hour.
4. Wash each well 3 times as in step 2.
5. Add 100 µL of 1×STP-HRP solution to each well, incubate at room temperature for 20 minutes.
6. Wash each well 4 times as described in step 2.
7. Add 100 µL of Substrate solution to each well, incubate at room temperature for 15 minutes. **Protect from light.**
8. Add 100 µL of Stop solution to each well, gently tap the plate frame for a few seconds to ensure thorough mixing.
9. Measure absorbance of each well at 450 nm immediately.

**CALCULATION**

1. Subtract the absorbance of the blank from that of standards and samples.
2. Generate a standard curve by plotting the absorbance obtained (y-axis) against mouse GDF-15 concentrations (x-axis). The best fit line can be generated with any curve-fitting software by regression analysis. Any curve of 4-parameter or log-log curve fitting can be used for calculation.


- Determine mouse GDF-15 concentration of samples from standard curve and multiply the value by the dilution factor.

**TYPICAL STANDARD CURVE**

The following standard curve is provided for demonstration only. A standard curve should be generated for each set of sample assay.

Mouse GDF-15 (pg/mL)	Absorbance (450 nm)	Blanked Absorbance
0	0.091	0
3.9	0.126	0.035
7.8	0.164	0.073
15.6	0.246	0.155
31.2	0.404	0.313
62.5	0.692	0.601
125	1.259	1.168
250	2.216	2.125

Mouse GDF-15 standard curve (4-parameter)

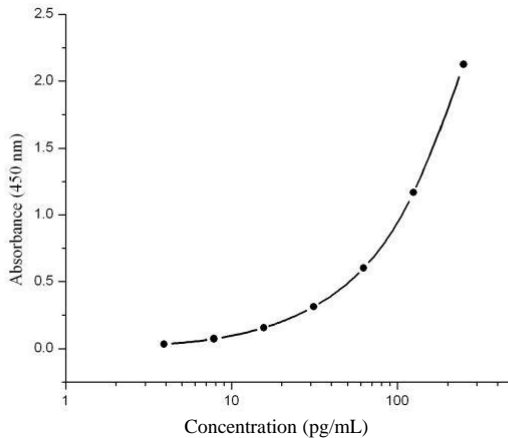

**ASSAY CHARACTERISTICS**

**A. Sensitivity**

The lowest level of mouse GDF-15 that can be detected by this assay is 3.9 pg/mL.

Website: [www.immunodiagnostics.com.hk](http://www.immunodiagnostics.com.hk)

E-mail: [info@immunodiagnostics.com.hk](mailto:info@immunodiagnostics.com.hk)(HK) /[info@immunodiagnostics.ca](mailto:info@immunodiagnostics.ca)(Canada) 4

Tel: +852 3502 2780 (HK) / +1-437-886-5136 (Canada)

**B. Precision**

Intra-assay Precision (Precision within an assay) C.V. <2.9%.

Inter-assay Precision (Precision between assays) C.V. <6.1%.

**REFERENCES**

1. Bootcov M. R., et al. (1997) *PNAS*; 94:11514-11519.
2. Welsh J.B., et al. (2003) *PNAS*;100:3410-3415.
3. Wang T. J, et al. (2012) *Circulation* 126; 1596– 1604.
4. Nair V., et al. (2017) *J.Am. Soc. Nephrol.* 28 2223-2240.
5. Hsu J-Y, et al. (2017) *Nature*; 550: 255-259.

**SUMMARY OF ASSAY PROCEDURE**

